

ANALIZA BIALEK



100014386

Laboratory of Analysis

Client: Peptidebestellung.de
Order number: 100014386
Name: Peptidebestellung.de BPC-157
Number of samples: 1 vial

Batch number: -----
Receive date: 2026-04-30
Start date: 2026-05-08
Enda date: 2026-05-11

Sample identification

Substance	Method of taking a sample	Form
BPC-157	Sample provided by customer	White powder in a glass vial


Results

Substance	Sample name	Content	Purity
BPC-157	Peptidebestellung.de BPC-157	10,60mg	99,43%
Endotoxin Level	Peptidebestellung.de BPC-157	3,11EU/vial	-----

Research comment

The test sample was applied in the amount of 3pl to the BioBasic 6 Thermo Scientific column. During the course of the analysis with the method a linear gradient in the solutions of H2O and Acetonitrile with the addition of 0.1% trifluoroacetic acid, a peak of the sought substance appeared. Its content, when compared to the reference chromatogram, is 10,60mg. Height the measurement error is + - 0,05mg. The actual state of the sample sent before the test is presented on the photo below

Photo of the test sample

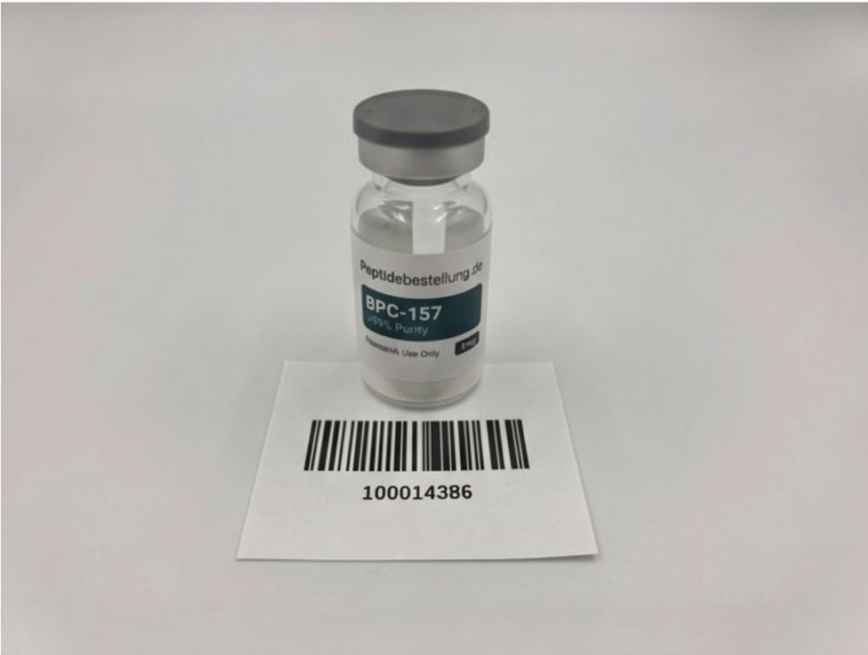

Password

L4B9S2W

Analiza Biatek sp. z o.o.
KRS: 0000966188
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul, Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zajac